


JuggerKnot™

SOFT ANCHOR

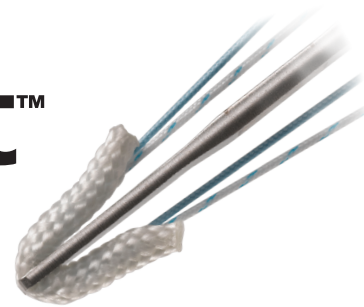

It's small. It's strong.
And it's all suture...

JuggerKnot™ Soft Anchor–2.9mm is designed for multiple indications, including rotator cuff repairs!



Small

- 47% smaller diameter than 5.5mm suture anchor
- Able to place anchors in locations not previously possible with larger anchors

Strong

- Pullout strength approximately 120–140 lbs.^{1*}
- Pullout strength is equivalent to the large 5.0mm Ti Corkscrew® anchor¹
- Pullout strength is significantly stronger when compared to competitive anchors^{1**}

Suture Configuration

- Soft sleeve braided construct provides solid cortical fixation
- Implant made from 2.0mm diameter polyester braid
- Double loaded with #2 MaxBraid™ suture
- Eliminates the possibility of rigid material loose bodies in the joint

The JuggerKnot™ Soft Anchor represents the next generation of suture anchor technology for rotator cuff. The 2.9mm deployable anchor design is completely suture-based, and is the first of its kind.

With over 50,000 anchors sold, the award winning JuggerKnot™ Soft Anchor's new configuration includes a suture sleeve double-loaded with #2 MaxBraid™ sutures, a drill guide and drill bit to simplify insertion.



¹ Testing of this anchor was performed in bone block.

^{**} PushLoc™ Anchor 2.9mm, Gryphon™ Anchor 3.0mm, and BioRaptor™ Anchor 3.0mm

All trademarks herein are the property of Biomet, Inc. or its subsidiaries unless otherwise indicated.

PushLoc™ is a trademark of Arthrex

Corkscrew® and Gryphon™ are trademarks of DePuy Mitek.

BioRaptor™ is a trademark of Smith and Nephew.

This material is intended for the sole use and benefit of the Biomet sales force and physicians. It is not to be redistributed, duplicated or disclosed without the express written consent of Biomet.

For product information, including indications, contraindications, warnings, precautions and potential adverse effects, see the package insert and Biomet's website.

BIOMET®
SPORTS MEDICINE

The JuggerKnot™ Soft Anchors are intended for soft tissue to bone fixation for the following indications:

Shoulder Indications

- Bankart lesion repair
- SLAP lesion repair
- Acromio-clavicular repair
- Capsular shift/capsulolabral reconstruction
- Deltoid repair
- Rotator cuff tear repair
- Biceps tenodesis

Elbow Indications

- Ulnar or radial collateral ligament reconstruction
- Lateral epicondylitis repair
- Biceps tendon reattachment

Hip Indications

- Acetabular labral repair

Knee Indications


- Extra-capsular repair: MCL, LCL, and posterior oblique ligament
- Iliotibial band tenodesis
- Patellar tendon repair
- VMO advancement
- Joint capsule closure

Foot and Ankle Indications


- Medial/lateral repair and reconstruction
- Mid- and forefoot repair
- Hallux valgus reconstruction
- Metatarsal ligament/tendon repair or reconstruction
- Achilles tendon repair

The JuggerKnot™ Soft Anchor-2.9mm also has indications in the Hand and Wrist: Collateral ligament repair, Scapholunate ligament reconstruction, Tendon transfers in phalanx, Volar plate reconstruction.

Pull-out Strength in Cadaver Bone¹

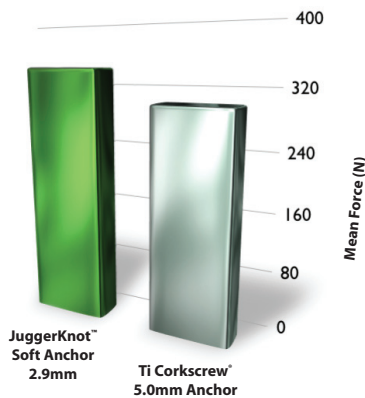

Pull-out Strength in Porcine Bone¹

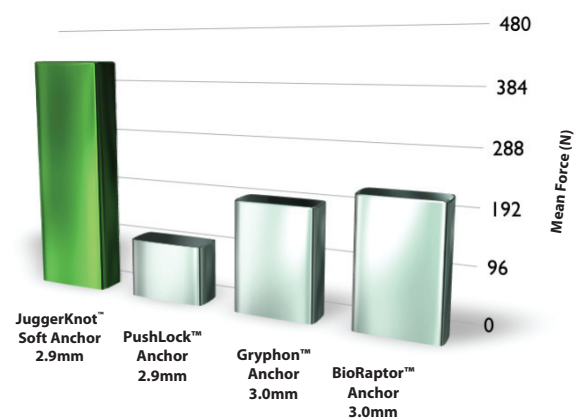

Ordering Information

JuggerKnot™ Soft Anchor–2.9mm

912050	Single
912060	10 pk.
912057	Disposable Instrument Kit

JuggerKnot™ Soft Anchor–2.9mm (Reusable¹)

912090	Guide
912091	Drill Bit
912092	Obturator
912093	Trocar

1. Data on file at Biomet Sports Medicine, Inc. Bench test results are not necessarily indicative of clinical results.

All trademarks herein are the property of Biomet, Inc. or its subsidiaries unless otherwise indicated.

This material is intended for the sole use and benefit of the Biomet sales force and physicians. It is not to be redistributed, duplicated or disclosed without the express written consent of Biomet.

For product information, including indications, contraindications, warnings, precautions and potential adverse effects, see the package insert and Biomet's website.

BIOMET[®]
SPORTS MEDICINE
One Surgeon. One Patient.™

P.O. Box 587, Warsaw, IN 46581-0587 • 800.348.9500 ext. 1501
©2011 Sports Medicine • www.biometSPORTSMEDICINE.com
Form No. BSM0298.0 • REV103111

www.biometSPORTSMEDICINE.com